



## ORIGINAL ARTICLE / ОРИГИНАЛНИ РАД

# Histological evaluation of tissue reactions to newly synthesized calcium silicate- and hydroxyapatite-based bioactive materials – *In vivo* study

Vanja Opačić-Galić<sup>1</sup>, Violeta Petrović<sup>1</sup>, Vukoman Jokanović<sup>2</sup>, Slavoljub Živković<sup>1</sup>

<sup>1</sup>University of Belgrade, Faculty of Dental Medicine, Department for Restorative Dentistry and Endodontics, Belgrade, Serbia;

<sup>2</sup>University of Belgrade, Vinča Institute of Nuclear Sciences, Belgrade, Serbia

## SUMMARY

**Introduction/Objective** Development of materials which could be used as biological bone substitutes is one of the most valuable and active fields of biomaterial research.

The goal of the study was to research the reaction of tissue on calcium silicate- (CS) and hydroxyapatite-based (CS-HA) newly synthesized nanomaterials, after being implanted into the subcutaneous tissue of a rats and direct pulp capping of rabbit teeth.

**Methods** The tested materials were implanted in 40 Wistar male rats, sacrificed after seven, 15, 30, and 60 days. The direct pulp capping was performed on the teeth of rabbits. Cavities were prepared on the vestibular surface of the incisors. The animals were sacrificed after 10 and 15 days. The control material was mineral trioxide aggregate (MTA). Histological analysis covered the tracking of inflammatory reaction cellular components, presence of gigantic cells, and necrosis of the tissue.

**Results** Seven days after the implantation, the strongest inflammatory response was given by the MTA ( $3.3 \pm 0.48$ ), while CS and CS-HA scored  $3 \pm 0.71$ . After 60 days, the rate of inflammatory reactions dropped, which was the least visible with CS-HA ( $0.2 \pm 0.45$ ). The least visible inflammatory reaction of the rabbits' pulp tissue was spotted with the CS ( $1.83 \pm 0.75$ ), than with the MTA and CS-HA ( $2.67 \pm 1.53$ ,  $3 \pm 0.63$ ).

**Conclusion** The newly synthesized materials caused a slight reaction of the subcutaneous tissue. CS-HA showed the best tissue tolerance. Nanostructural biomaterials caused a slight to moderate inflammatory reaction of the rabbits' pulp tissue only in the immediate vicinity of the implanted material.

**Keywords:** biocompatibility; calcium silicate system; hydroxyapatite; mineral trioxide aggregate

## INTRODUCTION

Biocompatibility of dental materials and the constraints imposed by their toxicity in contact with dental and other oral tissues are an important segment in the research of the newly synthesized materials. Cytotoxicity of the material can cause inflammatory reaction in contact with the surrounding tissue, significantly affecting the therapy outcomes [1, 2]. Therefore, multiple testing of synthesized materials is required in order to ensure their reliable application in day-to-day clinical practice. For many years now, the scientific community has been focusing on the need to evaluate the biological properties of new materials at the pre-clinical stage by using various *in vitro* and *in vivo* methods, as these mostly remain in long-term contact with local cells and tissues [3]. In this interaction, the onset of the foreign body reaction usually takes place immediately after the material is implanted (going through the stages of inflammation and healing, and involving a number of different cell types), making the *in vivo* biocompatibility testing one of the most important steps towards their prospective clinical application.

While the evaluation made based on *in vitro* assays may be faster in rendering biological in-

teraction data, the reliability of such data remains questionable compared to the data obtained in more complex *in vivo* conditions. *In vivo* assays are normally carried out on animal models (implantation in subcutaneous, muscle, bone, or other tissues), and they precede assays on target animal tissues and human clinical trials [4].

Subcutaneous tissues are tissues of choice for the biocompatibility evaluation of the implanted material. In the opinion of the authors they are found on highly accessible sites, enabling the evaluation of the biological reactions to biomaterials or, in other words, facilitating detection of inflammatory tissue reactions to the agents in the implanted material [3]. Histological examination is the most frequently used method in the research of tissue compatibility and its capability to restrict the inflammatory reaction to the implanted material [5–9].

The direct pulp capping is a therapeutic procedure for preserving the dental pulp vitality by covering the exposed pulp injury with materials that will foster reparative dentine formation [10]. The direct capping material plays a key role in the course of this treatment as it comes into direct contact with the pulp tissue. Although calcium hydroxide has been a direct pulp capping

Received • Примљено:  
July 19, 2016

Accepted • Прихваћено:  
October 4, 2016

Online first: March 10, 2017

## Correspondence to:

Vanja OPAČIĆ GALIĆ  
Department for Restorative  
Dentistry and Endodontics,  
Faculty of Dental Medicine  
Rankeova 4  
11000 Belgrade, Serbia  
[vanja.opacic.galic@gmail.com](mailto:vanja.opacic.galic@gmail.com)

agent in most frequent and longest use [10, 11, 12], the practice of many years has also shown frequent unforeseeable outcomes of this therapy [13, 14]. In the era of regenerative endodontics, new procedures and materials for biological therapy and tooth revitalization have been introduced, including biomaterials such as calcium phosphate, calcium silicate, and bioactive glass-ceramic cements. These bioactive dental materials are essential for a better and more effective regenerative endodontic treatment [15].

The objective of this study was to investigate the tissue inflammatory response to newly synthesized nanomaterials based on calcium silicates (CS) and hydroxyapatite (CS-HA) in *in vivo* conditions by a) implanting the material into the subcutaneous tissue of rats, and b) direct capping of exposed dental pulp of rabbits.

## METHODS

Permission for the experimental work on animals was obtained from the Ethical Committee of the Belgrade University Faculty of Dental Medicine (No. 36/5, April 4, 2012). The experiment was conducted in line with the international standards ISO 7405 and ISO 10993-2 (animal welfare requirements) [16, 17]. The initial step in carrying out this study was an innovative method of bio-ceramic material synthesis (with nanoscale particles) applied for the first time by V. Jokanović. The materials used in this study were nanostructured CS with and without the addition of 40% HA-CS mixed with distilled water in the 2:1 ratio of powder to water, according to the recommended protocol. The control material was mineral trioxide aggregate (ProRoot MTA, Dentsply Maillefer, Ballaigues, Switzerland) mixed in a 3:1 ratio, according to the instructions of the manufacturer.

### Design of the subcutaneous implantation experiment

Forty male rats (Wistar albino), between 2.5 and 3 months old and weighing on average 350 g each, were used. After the animals were anaesthetized, two-centimeter-long incisions in the animals' backs were made in the head-to-tail direction. Using the blunt dissection to the right and left of the spine, two pockets approximately 15 mm deep were opened and sterile polyethylene tubes with the test materials were implanted using sterile clinical tweezers. Polyethylene tubes 10 mm long and with internal diameter of 1 mm, half-filled with freshly mixed materials (CS, CS-HA, and MTA) were implanted in the subcutaneous tissue. The empty half of the tube was used as the negative control. Each animal received two tube implants. The tube with the test material was inserted on the right side of the spine and the tube with MTA on the left. The tubes were positioned so that the material was at all times oriented towards the head, and the empty half of the tube towards the tail. By random selection the animals were divided into two groups of 20 for each tested material. Ten animals (five of each material) were sacrificed in each of the four observation periods – days 7, 15, 30, and 60.

Tissue samples together with polyethylene tubes were fixed in 10% buffered formalin. Then the polyethylene tubes were removed. The tissue was then prepared for light microscopy in a standard way, involving dehydration in a series of ethanol solutions of increasing concentrations, illumination in xylol, and paraffin embedding. Paraffin samples 4 µm thick were stained in haematoxylin and eosin. Microscopic slides were analyzed in an optical microscope (BX-51, Olympus Corporation, Tokyo, Japan) and microphotographs were taken by a digital camera (CD video camera, Pixelink, Gloucester, Ontario, Canada) connected to a 19" PC screen (Dell Inc., Round Rock, TX, USA) [2].

In line with international standards (ISO 10993-6, Biological evaluation of medical devices – Part 6: Test for local effect after implantation), local tissue reactions where the materials had been implanted were evaluated. In the histological examination of the prepared samples, the parameters were analyzed qualitatively and semi-quantitatively (modified according to Scarparo et al. [6] and Lotfi et al. [18]): a) inflammatory response (0 – no inflammation; 1 – minimal (< 25 inflammatory cells); 2 – mild (26–50 inflammatory cells); 3 – moderate (51–100 inflammatory cells); 4 – severe (> 100 inflammatory cells); b) vascular congestion (0 – absent; 1 – minimal; 2 – mild; 3 – moderate; 4 – severe, involving blood vessel burst).

### Design of the direct pulp capping experiment

The animal model used in this experimental part of the study were four rabbits (*Oryctolagus cuniculus*) of both sexes, from different broods, aged about 12 months, average weight of 4 kg, on controlled diet and receiving daily care. For the purposes of the surgical procedure, the general dissociative anesthesia (xylazine, ketamine, acepromazine) was administered. The average duration of anesthesia was 100 minutes.

The surgical procedure was carried out in aseptic conditions and so as to ensure minimum trauma. Each tooth was cleaned, dried and disinfected (30% hydrogen peroxide and 5% iodine tincture). Class V cavities were then created in the gingival third of vestibular surfaces of incisors by using round, water-cooled diamond burs. A new set of diamond and carbide burs was used for each animal. In the middle of the cavity, pulp was exposed using sterile, round bur. Cavities were gently dried, with no pressure exerted, using sterile cotton wool balls. Freshly mixed material was applied to the exposed pulp. All cavities were closed with glass ionomer cement (GC FUJI VIII, GC Corporation, Tokyo, Japan) as a definitive filling. The material used for direct capping of the exposed pulp was MTA and it was implanted in the upper right maxillary incisor, while the other three incisors were implanted with CS and CS-HA, in two rabbits respectively. The animals were sacrificed after 10 and 15 days, by intravenous injections. Having removed soft tissues, the teeth in the alveoli were cut with a diamond disc. The samples were fixed in 10% formalin and decalcified. Following the decalcification, the tissue was fixed in semi-enclosed benchtop tissue processor (Leica TP1020, Leica Biosystems, Wetzlar, Germany) and

then embedded in paraffin blocks. Serial tissue sections 5  $\mu\text{m}$  thick (eight from each sample) were cut from the paraffin blocks. The slides were stained in haematoxylin and eosin, following the standard procedure.

The microscopic slides were examined by optical microscopy, using Olympus Cell-B software package and Olympus 5 microscope at magnifications of  $\times 10$ ,  $\times 40$ ,  $\times 100$ , and  $\times 200$ . In addition to the software, the pathohistological parameters were assessed qualitatively, semi-quantitatively, and quantitatively. Examination of every tooth included the scoring of the following parameters (scoring system 1–4): a) pulp inflammatory response: i) intensity (1 – no inflammation, 2 – mild, 3 – moderate, 4 – severe, > 25 inflammatory cells), ii) extent of inflammation (1 – no inflammation, 2 – mild, inflammatory cells close to the exposed portion of the pulp, 3 – moderate, inflammatory cells in the area of coronal pulp, 4 – severe, whole coronal pulp is infiltrated or necrotic), iii) general state of the pulp (1 – no inflammation, 2 – with inflammation, 3 – abscess, 4 – necrosis); b) other findings in the pulp (gigantic cells, direct capping material particles, presence of microorganisms).

In the statistical analysis, the non-parametric Kruskal–Wallis test with Dunn's post hoc test for inter-group comparisons was used. The statistical analysis was made using the Minitab 16 software package (Minitab Inc., State College, PA, USA).

## RESULTS

The results of the histological examination of subcutaneous implantation are shown in Table 1 and in Figures 1–6.

In the examined samples seven days after the implantation of CS and CS-HA, a moderate inflammatory reaction was observed (score 3) (Figure 1), while the connective tissue with the MTA implant showed somewhat more intensive inflammatory reaction (3.3) with diffuse and focal subcapsular and perivascular inflammatory infiltrates (Figure 2). Inflammatory infiltrate cells included lymphocytes and plasmocytes, while rare granulocytes were observed in only two samples. The connective tissue had a small number of normal-structure blood vessels with signs of moderate congestion, and it could receive scores 2.8 and 2.5 for CS and CS-HA, respectively, and score 2.4 for MTA.


In the observed slides 15 days after implantation of CS and CS-HA materials, mild inflammation was observed (scores 2 and 1.6, respectively) (Figure 3), while the MTA group displayed mild to moderate inflammation (score 2.3). Blood vessels were of the normal number and with signs of minimal venous stasis, receiving score of 0.8 in the CS-HA group, while the MTA and CS groups displayed minimal and mild congestion, respectively (scores 1.3 and 1.6, respectively).

In the observed samples 30 days after the implantation, the connective tissue was of normal structure and with minimal number of inflammatory cells in the CS and CS-HA groups (scores 1.6 and 1.4, respectively) (Figure 4). In the MTA group, the surrounding tissue in most samples showed signs of mild inflammation (score 1.9).


**Table 1.** Mean value of inflammation scores and standard deviation

Material	7 days	15 days	30 days	60 days
CS	3 $\pm$ 0.71	2 $\pm$ 0.71	1.60 $\pm$ 0.55	0.5 $\pm$ 0.58
CS-HA	3 $\pm$ 0.82	1.6 $\pm$ 0.55	1.40 $\pm$ 0.55	0.2 $\pm$ 0.45
MTA	3.3 $\pm$ 0.48	2.3 $\pm$ 1.06	1.90 $\pm$ 0.88	0.44 $\pm$ 0.73
Control	2.5 $\pm$ 1.43	1.9 $\pm$ 0.74	1.50 $\pm$ 0.53	0.67 $\pm$ 1


CS – calcium silicates; CS-HA – calcium silicate with hydroxyapatite; MTA – mineral trioxide aggregate

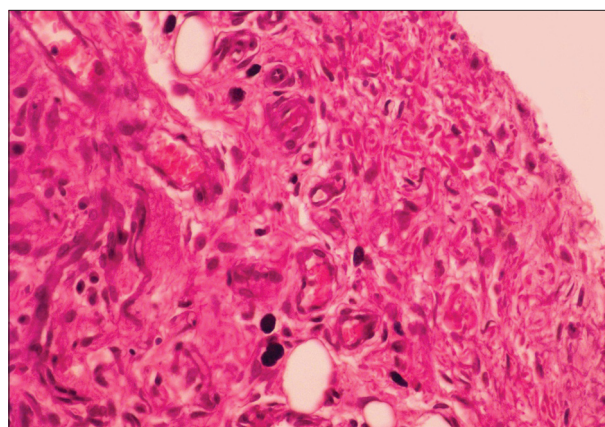


**Figure 1.** Calcium silicate implantation after seven days; mild inflammatory reaction is visible, while rare monocytes, lymphocytes, and granulocytes can be found in infiltrate; blood vessels with signs of moderate congestion (H&E,  $\times 40$ )

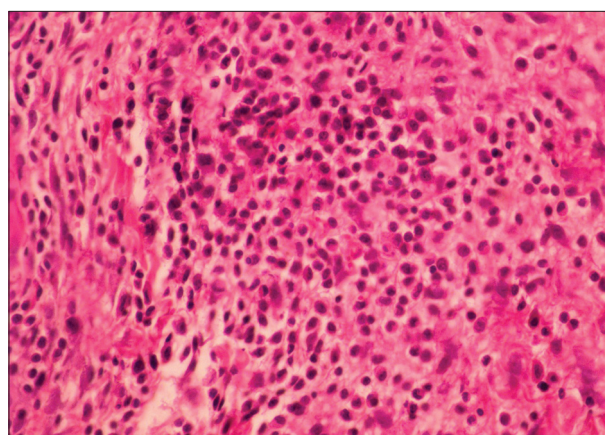


**Figure 2.** Mineral trioxide aggregate implantation after seven days; visible focal and diffuse inflammatory reaction of connective tissue (H&E,  $\times 40$ )

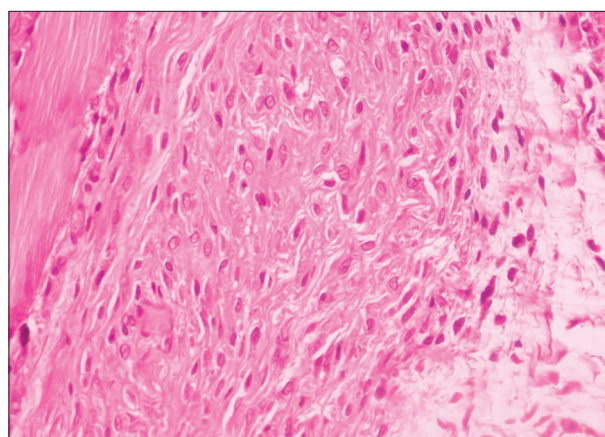


**Figure 3.** Calcium silicate implantation after 15 days; connective tissue of mostly preserved integrity is visible, no venous stasis (score 1.4); presence of lymphocytes and plasmacytes confirms chronically inflammatory reaction (H&E,  $\times 40$ )

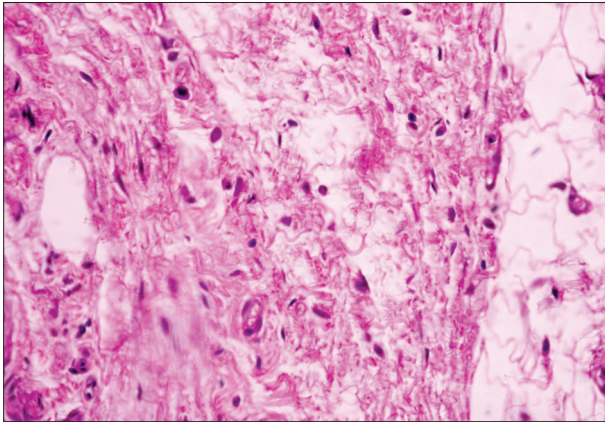

**Figure 4.** Calcium silicate implantation after 30 days; integrity of the connective tissue is visible, with minimal number of inflammatory infiltrate cells (score 0.6) (H&E, ×40)

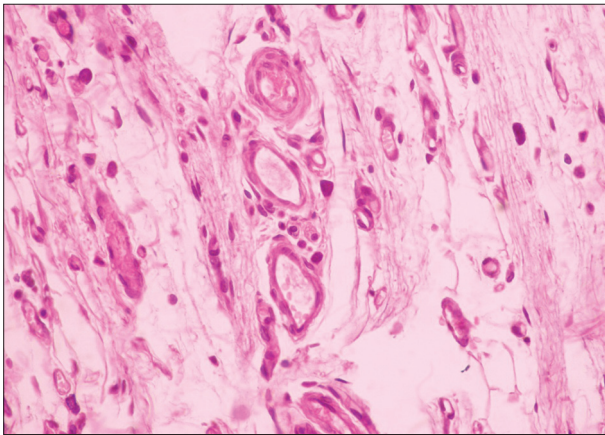

**Figure 5.** Calcium silicate implantation after 60 days; loose connective tissue with preserved integrity is visible; single cells of inflammatory infiltrate are present (score 0.5) as well as an increased number of new blood vessels, which indicates tissue remodeling (H&E, ×40)

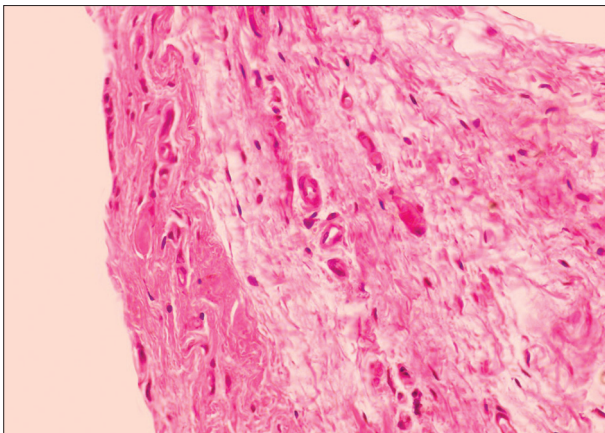


**Figure 6.** Hydroxyapatite-based implantation after 60 days; subcapsular connective tissue with preserved integrity (score 0) is visible (H&E, ×40)

The connective tissue was with a usual number of blood vessels and no signs of venous congestion, receiving score 0.6 in the CS and CS-HA groups, and score 0.8 in the MTA group.


In the tested samples, 60 days after the beginning of the experiment, loose connective tissue with individual cells of inflammatory infiltrate could be observed [score

**Table 2.** Mean inflammation score values of the tested materials

Material	Intensity	Extent	General state of the pulp
CS	1.83 ± 0.75	2.17 ± 0.75	1.5 ± 0.55
CS-HA	3 ± 0.63	2.17 ± 0.41	2.17 ± 0.41
MTA	2.67 ± 1.53	2.67 ± 1.15	2.67 ± 1.15

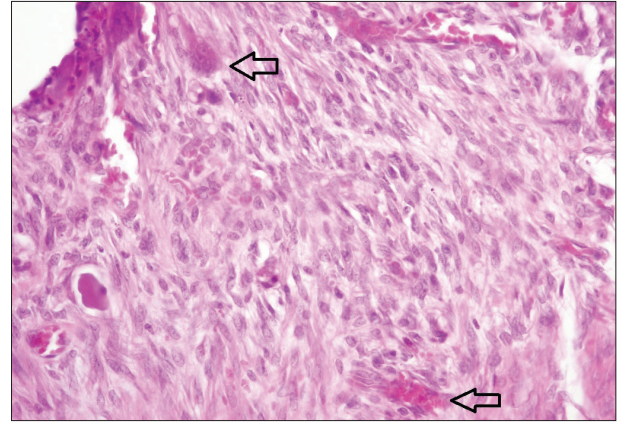

**Figure 7.** Direct pulp capping with calcium silicate; reactive chronic inflammation with rare mononuclear cells and focally present giant type cells around the foreign body (arrows) (H&E, ×400)

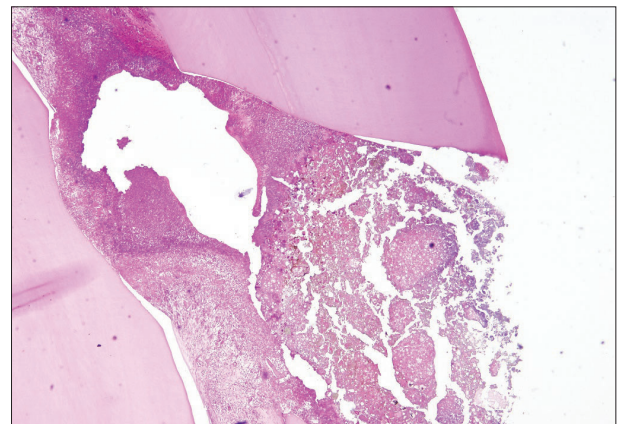


**Figure 8.** Direct pulp capping with hydroxyapatite; tooth enamel cavity; implanted material surrounded with mild to intensive pulp inflammatory reaction with focal necrosis (H&E, ×40)

0.4 for CS-HA and MTA) (Figure 6) and score 0.5 for CS (Figure 5)]. The blood vessels of normal structure and in a normal number, with no signs of venous stasis observed in any of the tested material (0).


The histological examination results of the rabbit teeth direct pulp capping are shown in Table 2 and Figures 7–11.

The pulp tissue below the CS material showed signs of mild inflammatory reaction (Figure 7). The general state of the pulp suggested a mild inflammatory reaction (score 2). While the difference between the tested materials (CS and CS-HA) was not statistically significant, it was significant between CS and MTA ( $p = 0.040$ ).


All the observed samples where CS-HA was used as the direct capping material showed signs of moderate inflammation (Figure 8). The general state of the pulp inflammation received a score of 2. A significant number of gigantic cells and scattered particles of the material were observed in the samples (Figure 9), which was statistically

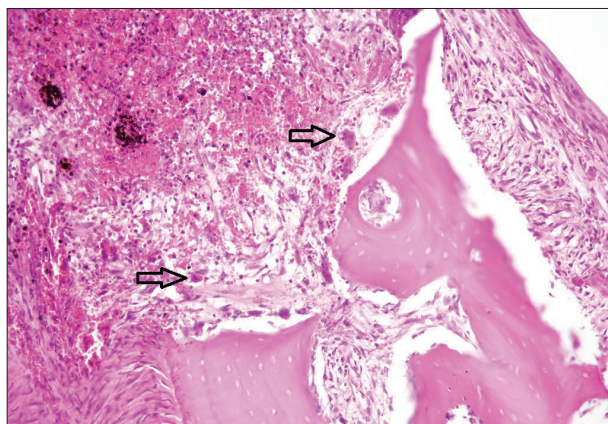

**Figure 9.** Loose particles of hydroxyapatite visible in pulp tissue surrounded with giant type cells around the foreign body (arrows) (H&E,  $\times 200$ )

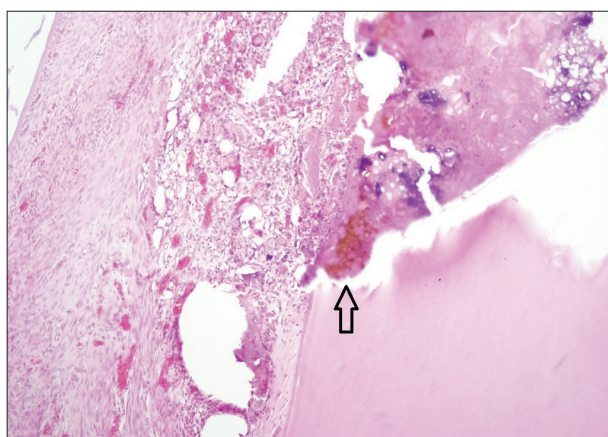

**Figure 10.** Direct pulp capping with mineral trioxide aggregate; necrotic zones spread around the mineral trioxide aggregate particles; blood vessels show signs of acute hyperemia (H&E,  $\times 100$ )

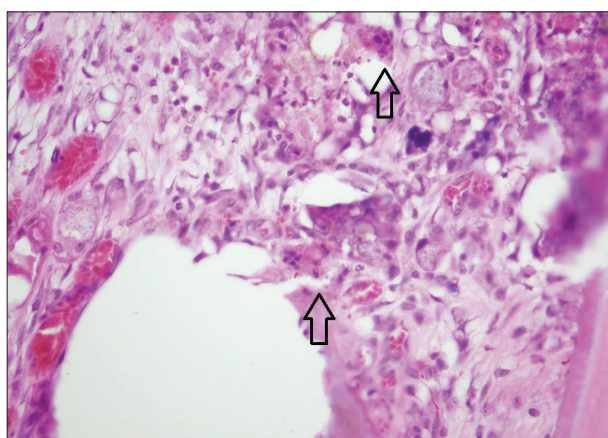

**Figure 11.** Direct pulp capping with mineral trioxide aggregate; mild inflammatory reaction with phagocytized material, a number of foamy histiocytes and giant type cells around the foreign body (arrows) (H&E,  $\times 400$ )

significant in the CS ( $p = 0.001$ ) and MTA groups ( $p = 0.033$ ). No bacteria were detected in any of the samples.

All the samples with MTA as the direct capping material showed signs of mild to moderate inflammation, with a few inflammatory cells immediately around the site of the exposed pulp. An intensive inflammatory reaction was detected in one sample, where inflammatory cells infiltration throughout the coronal pulp and necrosis were

present (Figure 10). The presence of a small number of gigantic cells was detected in two samples; the particles of the phagocytized material were also observed (Figure 11). No bacteria were detected in any of the samples.

## DISCUSSION

At present, enormous progress has been achieved in synthesizing a number of new materials used in clinical practice.

The materials tested in this study were newly synthesized nanomaterials based on tricalcium and dicalcium silicates and hydroxyapatites (CS and CS-HA). Their structure and biological properties were compared with those of MTA, which is the golden standard of tricalcium silicate cements.

Understanding the mechanism of interaction between biological fluids or cells and endodontic materials is key to assessing new materials used in diagnostics and therapy, and to avoiding materials' harmful reactions after their use [19]. Nanoparticles of different size and chemical structure typically get deposited in mitochondria, causing considerable structural damage due to the reactive oxygen species synthesis that leads to oxidative stress. Mitochondria are the main locations of reactive oxygen species production in a cell, which can result in the generation of a hydroxyl radical – one of the most potent oxidizing agents in nature. Oxidative stress is the most common cause of cell injury.

Nanostructured calcium silicates, CS and CS-HA (with particles in the range of 117–477 nm), in the initial in vitro assays designed to assess genotoxicity and cytotoxicity showed the absence of harmful cell effects within the parameters of the Comet and the MTT assays [20, 21].

In vitro studies are fundamentally different from in vivo ones where proteins, tissue fluids, and other factors can reduce the toxic effects of the material [22]. In vivo assays render more comprehensive and clinically more relevant information about the tissue response over a protracted time period. The soft tissues' histological reaction to biomaterial has been a long established and frequently used method of biocompatibility assessment [7, 9]. These assays are highly reliable in evaluating the tissue irritation, and the interaction of tissue and biomaterial. Tissue reaction to an implant is a cumulative pathophysiological consequence of a) the healing of an acute injury sustained due to a surgical wound and the presence of implant, b) possible chronic inflammation, c) the surrounding tissue repair while adapting to the implant.

This experiment monitored short-term, but also long-term, effects of the materials on the tissue, since these data are relevant to the clinical use of the endodontic materials.

Monitoring of a specific response to a foreign body following the material implantation starts with *inflammation*, continuing through the stages of *wound healing* with the involvement of various cell types being specific indicators of the tissue repair stage. With the inflammatory process attenuating, the total number of inflammatory cells decreases while the wound healing process moves towards formation of granulation tissue and *fibrous encapsulation* of the implanted material.

The tissue surrounding the tested bioceramic materials (CS, CS-HA) showed the highest level of inflammation in the first 15 days, with moderate disruption in the connective tissue structures. The connective tissue around the MTA showed signs of the most severe inflammatory reaction with diffuse and focal subcapsular and perivascular infiltrates, which was evaluated as moderate and severe inflammation. Other researchers also reported such a powerful tissue response, observing even coagulative necrosis and dystrophic calcifications [7]. A number of factors initially caused such a severe inflammatory reaction to MTA. High pH values of the freshly mixed material, heat release upon setting, and stimulation of inflammatory cytokines (interleukin 1 and interleukin 6) contribute to such a powerful tissue response to MTA [18, 23, 24].

Tissue reaction to empty tubes (negative control) in this experiment is similar to findings reported by other researchers [9, 22, 24]. It was most severe on the seventh and the 15th day, with cellular infiltrate dominated by lymphocytes and plasmocytes, which is indicative of a chronic inflammatory reaction. The gigantic cells detected in some sites suggest the tissue's reaction to a foreign body. This reaction could partly be a result of surgical trauma sustained upon implanting the tubes in the tissue. At the end of weeks four and eight, the inflammatory infiltrate cells were disappearing, and the tissue at the point of contact with the tube was encapsulated. This suggests the body's capacity to contain the inflammatory reaction thus preventing further tissue damage, as confirmed in papers by Sumer et al. [5] and Scarparo et al. [6].

Further into the tissue repair process (after 30 and 60 days), significant decrease in the inflammation intensity, disappearance of inflammatory infiltrate cells, but also tissue repair and remodeling were observed in all tested materials. The inflammatory response after four and eight weeks of the experiment can be explained by inducing the release of proinflammatory cytokines by released particles of the hydroxyapatite layer formed on the surface of the bioceramic materials. This also suggests good interaction between the material and the cells from the surrounding tissue, which is a sign of good biocompatibility of the materials.

The pulp tissue response to the implanted material usually starts with an acute inflammation, which needs not be present in all cases [25]. The topography and chemistry of the surface of newly synthesized materials plays an important role in odontoblast adhesion to biomaterial. It is a known fact that micro- and nanotopography of the surface and adsorbed proteins have direct influence on the cell behavior and activity, primarily with respect to their adhesion and retention at the point of application [26].

Nanostructured CS cements show increased osteoblast adhesion, proliferation, and differentiation, since the bone itself has nanostructure, and the crystal size and geometry can modify the response of the surrounding tissue. The interaction between the direct capping material and the injured pulp tissue, and the ways in which the healing and repair processes are initiated and developed are still not fully clear. While many hypotheses exist, recent studies

have accorded the main role to growth factors in angiogenesis, mobilization of progenitor cells, differentiation, and, finally, biomaterial-assisted mineralization [27].

As a consequence of experimental perforation, but also of the initial effect of the tested materials, a mild to moderate inflammatory reaction was detected in all observed tooth samples. The inflammatory infiltrate was in close proximity of the implanted material and was not spreading further into the coronal pulp. The weakest inflammatory reaction, sporadically with total absence of inflammation, was observed in samples where CS cement was implanted as the direct capping material, which agrees with the findings of other researchers, who find up to 50% samples with no signs of inflammation in the early stage [12, 28]. Moderate inflammation was detected in the CS-HA and MTA samples, which is confirmed by similar experiments where inflammation appeared in more than 62% of the MTA samples after two weeks, with the intensity declining after eight weeks. This initially severe inflammatory response is a result of the pulp tissue coagulative necrosis in contact with MTA (pH being 9–10). This zone has a stimulating effect on the surrounding vital pulp tissue, which initiates a string of healing processes. Due to bio-degradation of the material in contact with the tissue fluids, Ca and P ions are released, creating alkaline environment, which has a favorable effect on adhesion and proliferation of cells involved in the healing processes [12, 29]. Asgary et al. [30] observed that new endodontic cements having similar structure as MTA but improved physical and chemical properties – they include the nanomaterials tested – show better pulp response (weaker inflammatory reaction) and thicker dentine bridge than MTA at a later stage.

Biomaterials are normally tested on animals, since they are a model of the environment one can find in humans. Nevertheless, animals are characterized by a huge range of differences with respect to anatomy, biochemistry, physiology, and other variables. In the absence of confirmation from human clinical trials, it is often difficult to draw a conclusion solely on the basis of animal testing. Testing carried out on live systems invariably leads to experimental variability. The more complex the system (human cells versus microorganism cells), the higher statistical variability of testing results can be expected [3].

## CONCLUSION

The results shown in the present *in vivo* study on the animal model have proven that the subcutaneous tissue of rats and the pulp tissue of rabbits have favorable biological response to newly synthesized nanostructured biomaterials (CS and CS-HA). The inflammatory reaction in the subcutaneous tissue was severe only in the initial days after the implantation and its intensity declined as a function of time. In direct pulp capping there was a mild to moderate inflammatory reaction in the close proximity of the implanted material. The tissues showed high tolerance to the implanted materials, which confirms their biocompatibility, as in previous *in vitro* studies.

## REFERENCES

- Camargo SE, Camargo CH, Hiller KA, Rode SM, Schweikl H, Schmalz G. Cytotoxicity and genotoxicity of pulp capping materials in two cell lines. *Int Endod J.* 2009; 42(3):227–37.
- Nedel F, Soki FN, Conde MCM, Zeitlin BD, Tarquinio SBC, Nör JE, et al. Comparative analysis of two colorimetric assays in dental pulp cell density. *Int Endod J.* 2011; 44(1):59–64.
- Raković D, Uskoković D. Biomaterijali. Beograd: Institut tehničkih nauka SANU, Društvo za istraživanje materijala Srbije; 2010. p. 221–40.
- Modareszadeh MR, Chogle SA, Mickel AK, Jin G, Kowsar H, Salamat N, et al. Cytotoxicity of set polymer nanocomposite resin root-end filling materials. *Int Endod J.* 2011; 44(2):154–61.
- Sumer M, Muglali M, Bodrumlu E, Guvenc T. Reactions of Connective Tissue to Amalgam, Intermediate Restorative Material, Mineral Trioxide Aggregate, and Mineral Trioxide Aggregate Mixed With Chlorhexidine. *J Endod.* 2006; 32(11):1094–96.
- Scarpato RK, Haddad D, Acasigua GA, Fossati AC, Fachin EV, Grecca FS. Mineral Trioxide Aggregate-based Sealer: Analysis of Tissue Reactions to a New Endodontic Material. *J Endod.* 2010; 36(7):1174–8.
- Parirokh M, Mirsoltani B, Raof M, Tabrizchi H, Haghdoost AA. Comparative study of subcutaneous tissue responses to a novel root-end filling material and white and grey mineral trioxide aggregate. *Int Endod J.* 2011; 44(7):283–9.
- Silva-Herzog D, Ramirez T, Mora J, Pozos AJ, Silva LAB, Silva RAB, et al. Preliminary study of the inflammatory response to subcutaneous implantation of three root canal sealers. *Int Endod J.* 2011; 44(5):440–6.
- Gomes-Filho JE, Watanabe S, Lodi CS, Cintra LT, Nery MJ, Filho JA, et al. Rat tissue reaction to MTA FILLAPEX. *Dent Traumatol.* 2012; 28(6):452–6.
- Zhang S, Yang X, Fan M. Bioaggregate, iRoot BP Plus optimize the proliferation and mineralization ability of human dental pulp cells. *Int Endod J.* 2013; 46(10):923–9.
- Ando Y, Honda MJ, Ohshima H, Tonomura A, Ohara T, Itaya T, et al. The induction of dentin bridge-like structures by constructs of subcultured dental pulp-derived cells and porous HA/TPC in porcine teeth. *J Med Sci.* 2009; 71(1-2):51–62.
- Zarrabi MH, Javidi M, Jafarian AH, Joushan B. Histologic Assessment of Human Pulp Response to Capping with Mineral Trioxide Aggregate and a Novel Endodontic Cement. *J Endod.* 2010; 36(11):1778–81.
- Roberts HW, Toth JM, Berzins DW, Charlton DG. Mineral trioxide aggregate material use in endodontic treatment: A review of the literature. *Dent Mater.* 2008; 24(2):149–64.
- Orhan EO, Maden M, Senguven B. Odontoblast-like cell numbers and reparative dentine thickness after direct pulp capping with platelet-rich plasma and enamel matrix derivative: a histomorphometric evaluation. *Int Endod J.* 2012; 45(4):317–25.
- Güven EP, Taşlı PN, Yalvac ME, Sofiev N, Kayahan MB, Sahin F. In vitro comparison of induction capacity and biomineralization ability of mineral trioxide aggregate and a bioceramic root canal sealer. *Int Endod J.* 2013; 46(12):1173–82.
- International Organization for Standardization. ISO 10993: 2009 ed.
- International Standard Organisation. ISO 7405 Dentistry-Preclinical Evaluation of Biocompatibility of Medical Device Used in Dentistry-Test method for Dental Material. Geneva, Switzerland; 1997.
- Lotfi M, Vosoughhosseini S, Saghiri MA, Mesgariabbasi M, Ranjkesh B. Effect of White Mineral Trioxide Aggregate Mixed With Disodium Hydrogen Phosphate on Inflammatory Cells. *J Endod.* 2009; 35(5):703–5.
- Fenoglio I, Fubini B, Ghibaudi EM, Turci F. Multiple aspects of the interaction of biomacromolecules with inorganic surface. *Adv Drug Deliv Rev.* 2011; 63(13):1186–209.
- Opačić-Galić V, Petrović V, Živković V, Jokanović V, Nikolić B, Knežević-Vukčević J, et al. New nanostructural biomaterials based on active silicate systems and hydroxyapatite: characterization and genotoxicity in human peripheral blood lymphocytes. *Int Endod J.* 2013; 46(6):506–16.
- Petrović V, Opačić-Galić V, Živković S, Nikolić B, Danilović V, Miletić V, et al. Biocompatibility of new nanostructural materials based on active silicate systems and hydroxyapatite: in vitro and in vivo study. *Int Endod J.* 2015; 48(10):966–75.
- Yavari HR, Shahi S, Rahimi S, Shakouie S, Roshangar L, Abbasi MM, et al. Connective tissue reaction to white and gray MTA mixed with distilled water or chlorhexidine in rats. *Iranian Endod J.* 2009; 4(1):25–30.
- Camilleri J. A review of the methods used to study biocompatibility of Portland cement-derived materials used in dentistry. *Malta Medical Journal.* 2006; 18(3):9–14.
- Vosoughhosseini S, Lotfi M, Shabi S, Baloo H, Mesgariabbasi M, Saghiri MA, et al. Influence of White versus Gray Mineral Trioxide Aggregate on Inflammatory Cells. *J Endod.* 2008; 34(6):715–17.
- Leprince JG, Zeitlin BD, Tolar M, Peters OA. Interaction between immune system and mesenchymal stem cell in dental pulp and periapical tissues. *Int Endod J.* 2012; 45(8):689–701.
- Gandolfi MG, Ciapetti G, Perut F, Taddei P, Modena E, Rossi PL, et al. Biomimetic calcium-silicate cement aged in simulated body solutions. Osteoblast response and analyses of apatite coating. *J Appl Biomater Biomech.* 2009; 7(3):160–70.
- Laurent P, Camps J, About I. Biodentine induces TGF-β1 release from human pulp cells and early dental pulp mineralization. *Int Endod J.* 2012; 45(5):439–48.
- Da Silva GF, Guerreiro-Tanomaru JM, Sasso-Cerri E, Tanomaru-Filho M, Cerri PS. Histological and histomorphometrical evaluation of furcation perforations filled with MTA, CPM and ZOE. *Int Endod J.* 2011; 44(2):100–10.
- Accorinte Mde L, Holland R, Reis A, Bortoluzzi MC, Murata SS, Dezan E, et al. Evaluation of Mineral Trioxide Aggregate and Calcium Hydroxide Cement as Pulp-Capping Agents in Human Teeth. *J Endod.* 2008; 34(1):1–6.
- Asgary S, Eghbal MJ, Parirokh M, Ghanavati F, Rahimi H. A comparative study of histologic response to different pulp capping materials and a novel endodontic cement. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod.* 2008; 106(4):609–14.

## Хистолошке реакције ткива на новосинтетисане биоактивне материјале на бази калцијум-силикатних система и хидроксиапатита – *in vivo* студија

Вања Опачић-Галић<sup>1</sup>, Виолета Петровић<sup>1</sup>, Вукоман Јокановић<sup>2</sup>, Славољуб Живковић<sup>1</sup>

<sup>1</sup>Универзитет у Београду, Стоматолошки факултет, Клиника за болести зуба, Београд, Србија;

<sup>2</sup>Универзитет у Београду, Институт за нуклеарне науке Винча, Србија

### САЖЕТАК

**Увод/Циљ** Усавршавање материјала који би могли да се користе као биолошке замене кости једна је од најзначајнијих и најактивнијих области истраживања биоматеријала.

Циљ овог рада је био да се испита одговор ткива на новосинтетисане наноматеријале на бази калцијум-силикатних система (КС) и хидроксиапатита (КС-ХА) после имплантације у поткожно ткиво пацова и директног прекривања пулпе зуба кунића.

**Методe** У поткожно ткиво 40 вистар пацова су имплантирани тестирани материјали, а после 7, 15, 30 и 60 дана животиње су жртвоване. Директно прекривање пулпе је реализовано на зубима кунића. На вестибуларним површинама секутића препарисани су кавитети, а експонирана пулпа је прекривана тестираним материјалима. Животиње су жртвоване после 10 и 15 дана. Контролни материјал у оба експеримента је био минерални триоксидни агрегат (МТА).

Хистолошка анализа је обухватила праћење ћелијске компоненте запаљења, присуства гигантских ћелија и некрозе ткива.

**Резултати** Седам дана после супкутане имплантације најјачи запаљенски одговор дао је МТА ( $3,30 \pm 0,48$ ), док је за КС и КС-ХА он оцењен са  $3,00 \pm 0,71$ . После 60 дана дошло је до опадања знакова запаљења, које је било најмање изражено око КС-ХА ( $0,20 \pm 0,45$ ). Најмање изражена запаљенска реакција пулног ткива кунића уочена је код материјала КС ( $1,83 \pm 0,75$ ), затим код МТА и КС-ХА ( $2,67 \pm 1,53$ ,  $3,00 \pm 0,63$ ).

**Закључак** Новосинтетисани материјали су изазвали благу запаљенску реакцију поткожног ткива пацова, а КС-ХА је показао најбољу ткивну толеранцију. Наноструктурни биоматеријали КС и КС-ХА су узроковали благу до умерену запаљенску реакцију пулног ткива кунића само у непосредној близини имплантираног материјала.

**Кључне речи:** биокompatibilност; калцијум-силикатни систем; хидроксиапатит; минерал-триоксид агрегат